


# SHOULDER GENERAL INSTRUMENTS

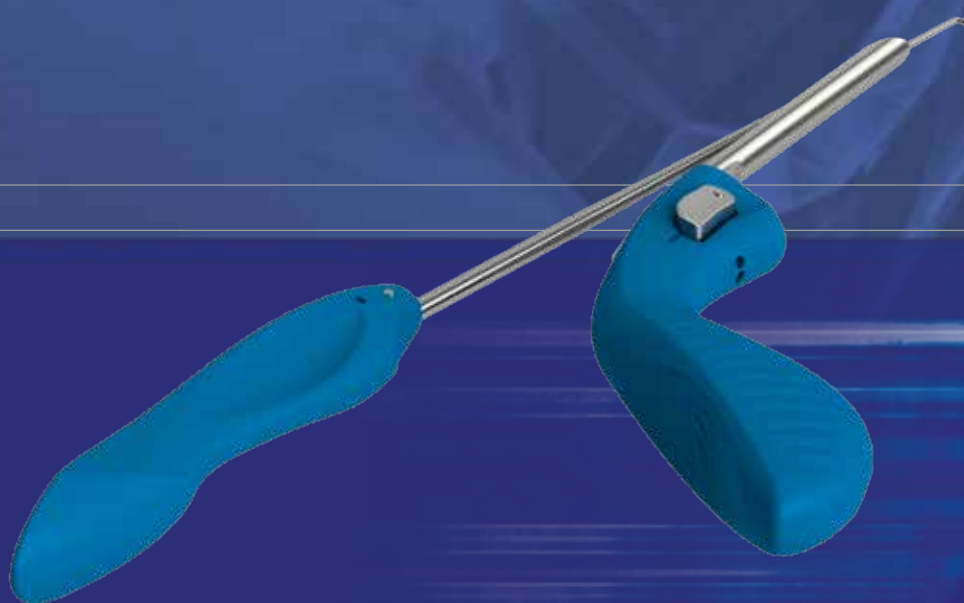

## Product Catalogue

Joint

Spine

Sports Med



## INDEX

<b>1. INSTRUMENTS OVERVIEW</b>	<b>4</b>
1.1 Probe (Ref. 05.10.10.0001)	4
1.2 Elevator (Ref. 05.10.10.0002)	4
1.3 Rasp (Ref. 05.10.10.0003)	4
1.4 Knot pusher (Ref. 05.10.10.0004)	4
1.5 V-Pipe	5
<b>2. INSTRUMENTS TRAY</b>	<b>6</b>

## 1. INSTRUMENTS OVERVIEW

Medacta's aim is to provide the surgeons a complete set of instruments that could be used during the arthroscopic treatment of the most common shoulder pathologies: torn or damaged labrum or ligaments, joint instability, torn tendons, loose bodies removal, arthroscopic treatment of inflammation phenomena, etc.

### 1.1 PROBE (Ref. 05.10.10.0001)

Designed to palpate soft tissues or the intra-articular structures during the arthroscopic procedures. It is provided with a 3mm tip with laser marking every 2mm on the tip and every 10mm along the shaft.

Tip 3 mm, straight shaft, lasermarking measures, WL 150 mm



### 1.2 ELEVATOR (Ref. 05.10.10.0002)

It is provided of a thin wedged tip to raise the tissues from the bone surface. It is designed with a bent tip (20°).

Bent thin tip 20°, Straight shaft, WL 150mm



### 1.3 RASP (Ref. 05.10.10.0003)

It is designed to rasp the bone surface during arthroscopic procedures. It is provided of a teathed tip bent upwards (20°).


Rasp tip bent upwards (20°), WL 150mm



### 1.4 KNOT PUSHER (Ref. 05.10.10.0004)

Designed with a spherical internal cavity to better accommodate the suture knot together with an atraumatic blunt tip.

Atraumatic blunt tip, spheric internal cavity, WL 150mm

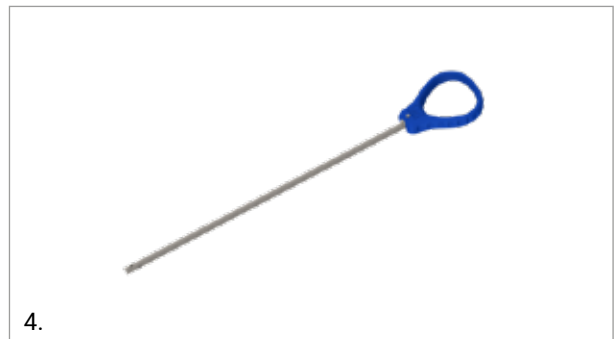

### 1.5 V-PIPE

Provided of atraumatic tip to avoid damage to soft tissues during the insertion into the arthroscopic portals. It is also designed with a V-Shape trail to better guide the tip of the instruments inside the portals. Available with rounded and reduced tips for easy insertion inside the portals. Combined with a dedicated detachable ergonomic handle with locking button.



#### V-Pipe Rounded tip (Ref. 05.10.10.0005)

Rounded atraumatic tip, internal V-shape, connection with detachable handle, WL 90mm



#### V-Pipe Reduced tip (Ref. 05.10.10.0006)

Reduced atraumatic tip, internal V-shape, connection with detachable handle, WL 90mm



#### V-Pipe detachable handle (Ref. 05.10.10.0007)

Ergonomic handle with locking button



## 2. INSTRUMENTS TRAY

Optional metal tray designed with dedicated brackets to contain all the instruments of the set.

References included (1 level tray)

### **SPORTS MEDICINE - SHOULDER GENERAL SET (05.10S.001)**

---



Ref.	Description	Qty.
05.10.10.0001	Probe	1
05.10.10.0002	Elevator	1
05.10.10.0003	Rasp	1
05.10.10.0004	Knot pusher	1
05.10.10.0005	V-Pipe rounded tip	1
05.10.10.0006	V-Pipe reduced tip	1
05.10.10.0007	V-Pipe handle	1

## NOTE FOR STERILISATION

The instruments are not sterile upon delivery. It must be cleaned before use and sterilised in an autoclave noting the regulations of the country, EU directives where applicable and following the instructions for use of the autoclave manufacturer. For detailed instructions please refer to the document "Recommendations for cleaning decontamination and sterilization of Medacta International orthopaedic devices" available at [www.medacta.com](http://www.medacta.com).



---

**REDEFINING BETTER  
IN ORTHOPAEDICS  
AND SPINE SURGERY**

---

MEDACTA.COM



**Medacta International SA**  
Strada Regina - 6874 Castel San Pietro - Switzerland  
Phone +41 91 696 60 60 - Fax +41 91 696 60 66  
info@medacta.ch

Find your local dealer at: [medacta.com/locations](https://www.medacta.com/locations)

All trademarks and registered trademarks are the property of their respective owners.  
This document is not intended for the US market.  
Please verify approval of the devices described in this document with your local Medacta representative.

Shoulder General Instruments  
Product Catalogue

ref: 99.106SMS.180  
rev. 01

Last update: May 2019