



916.939.3913

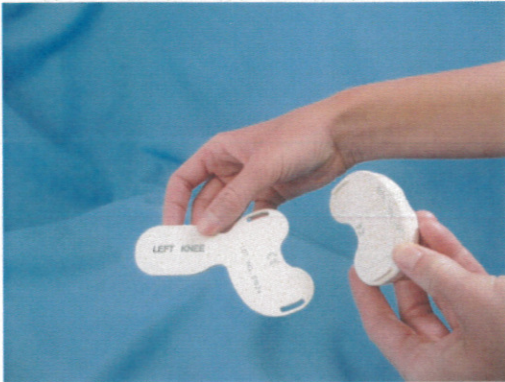

Conversion Plates 61-9312 and 61-9322 (Small and Large) are to be used in the event the Surgeon elects to use the Manual Libra Balancing System.

In that case, simply insert the selected eLIBRA Tibial Insert into the selected (Small or Large) Conversion Plate as shown.